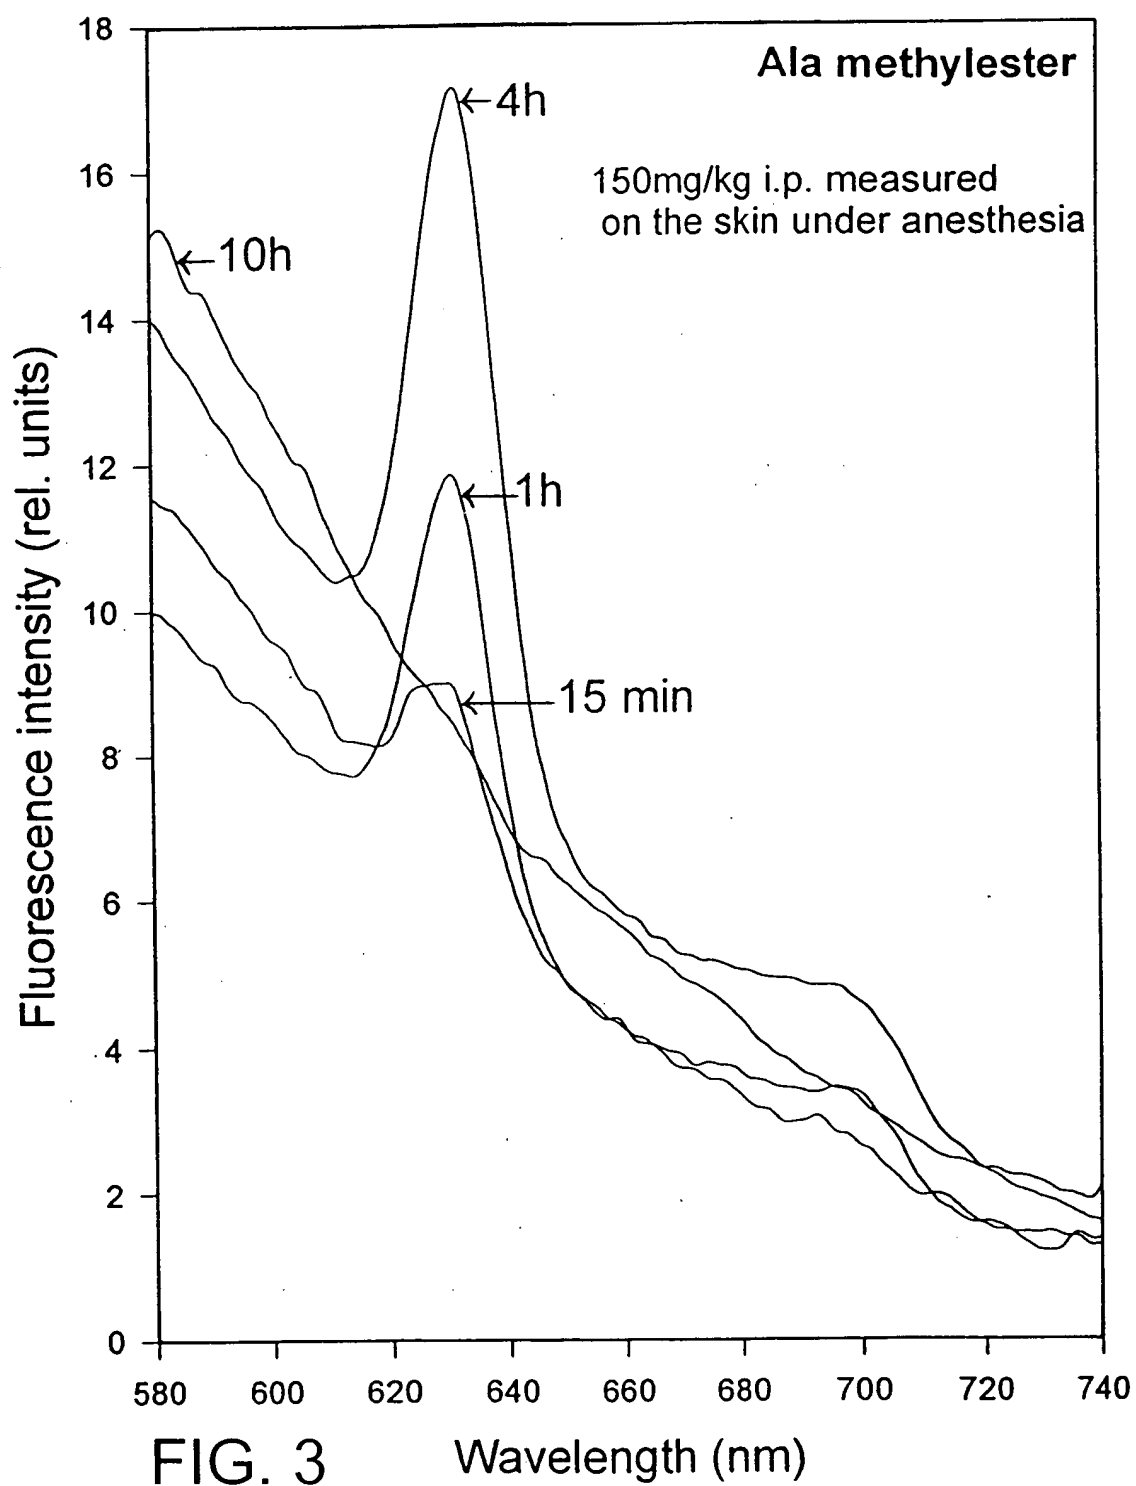


FIG. 2



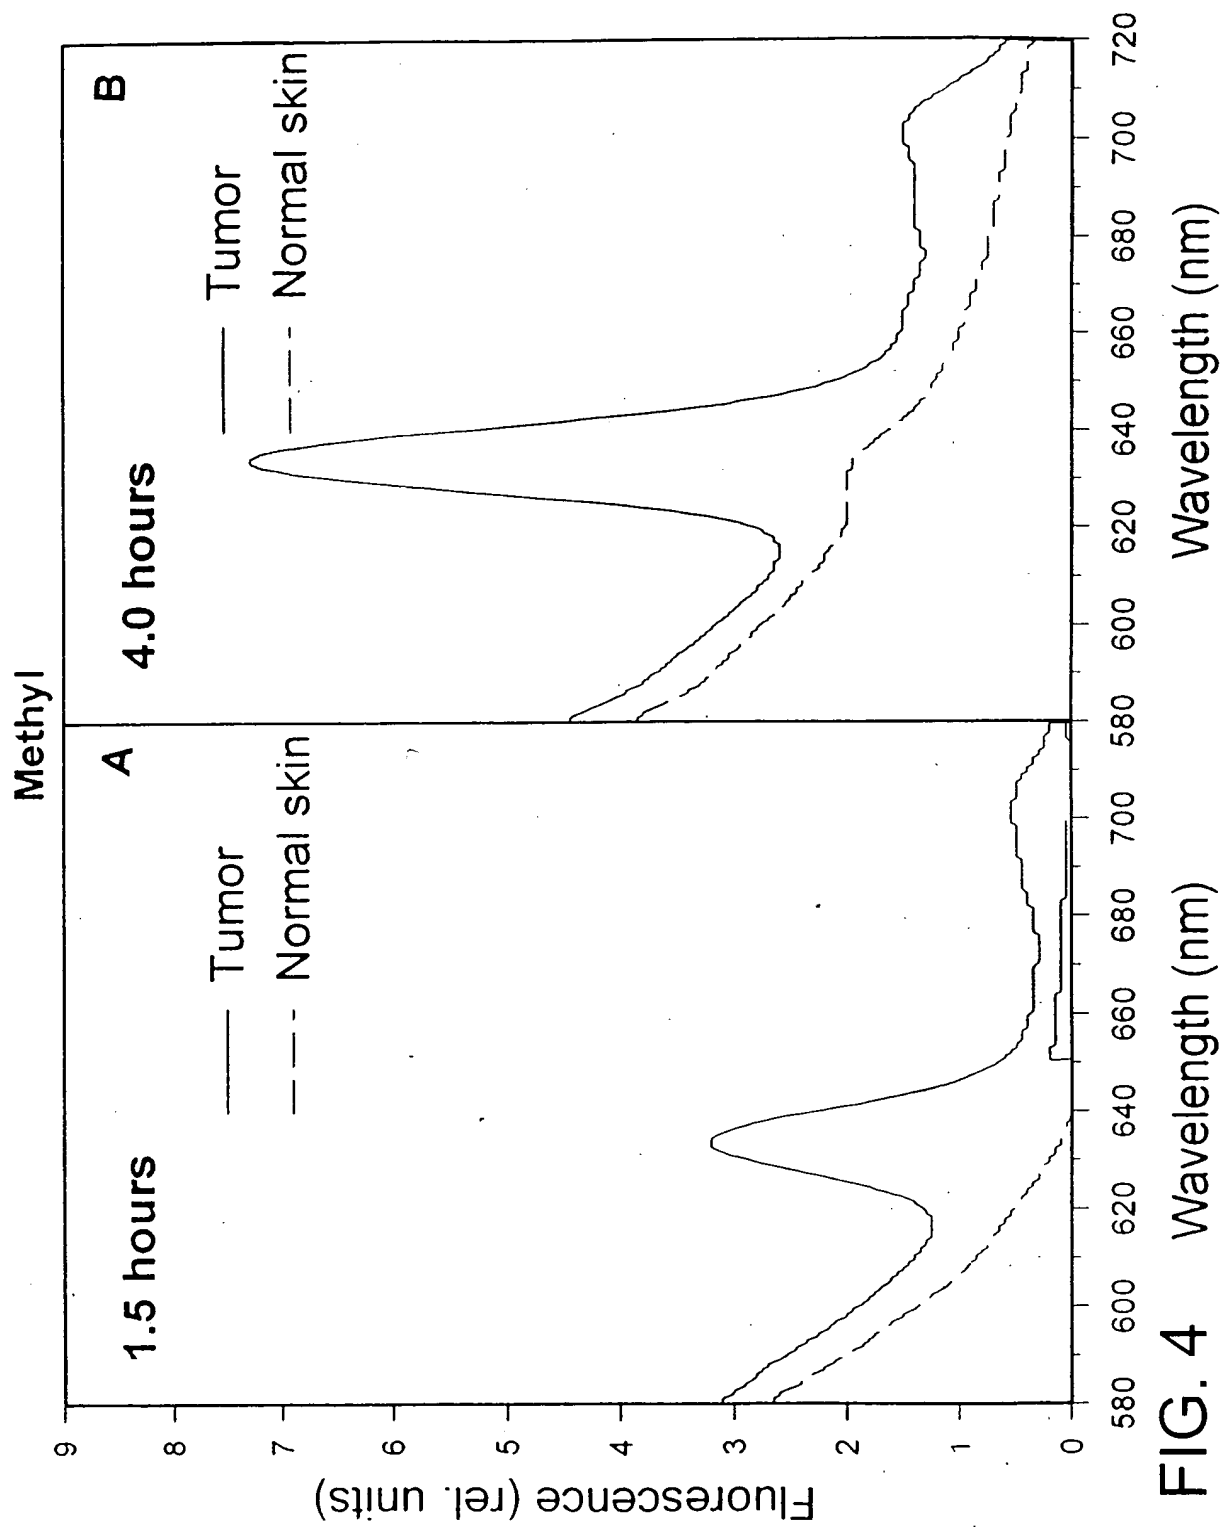
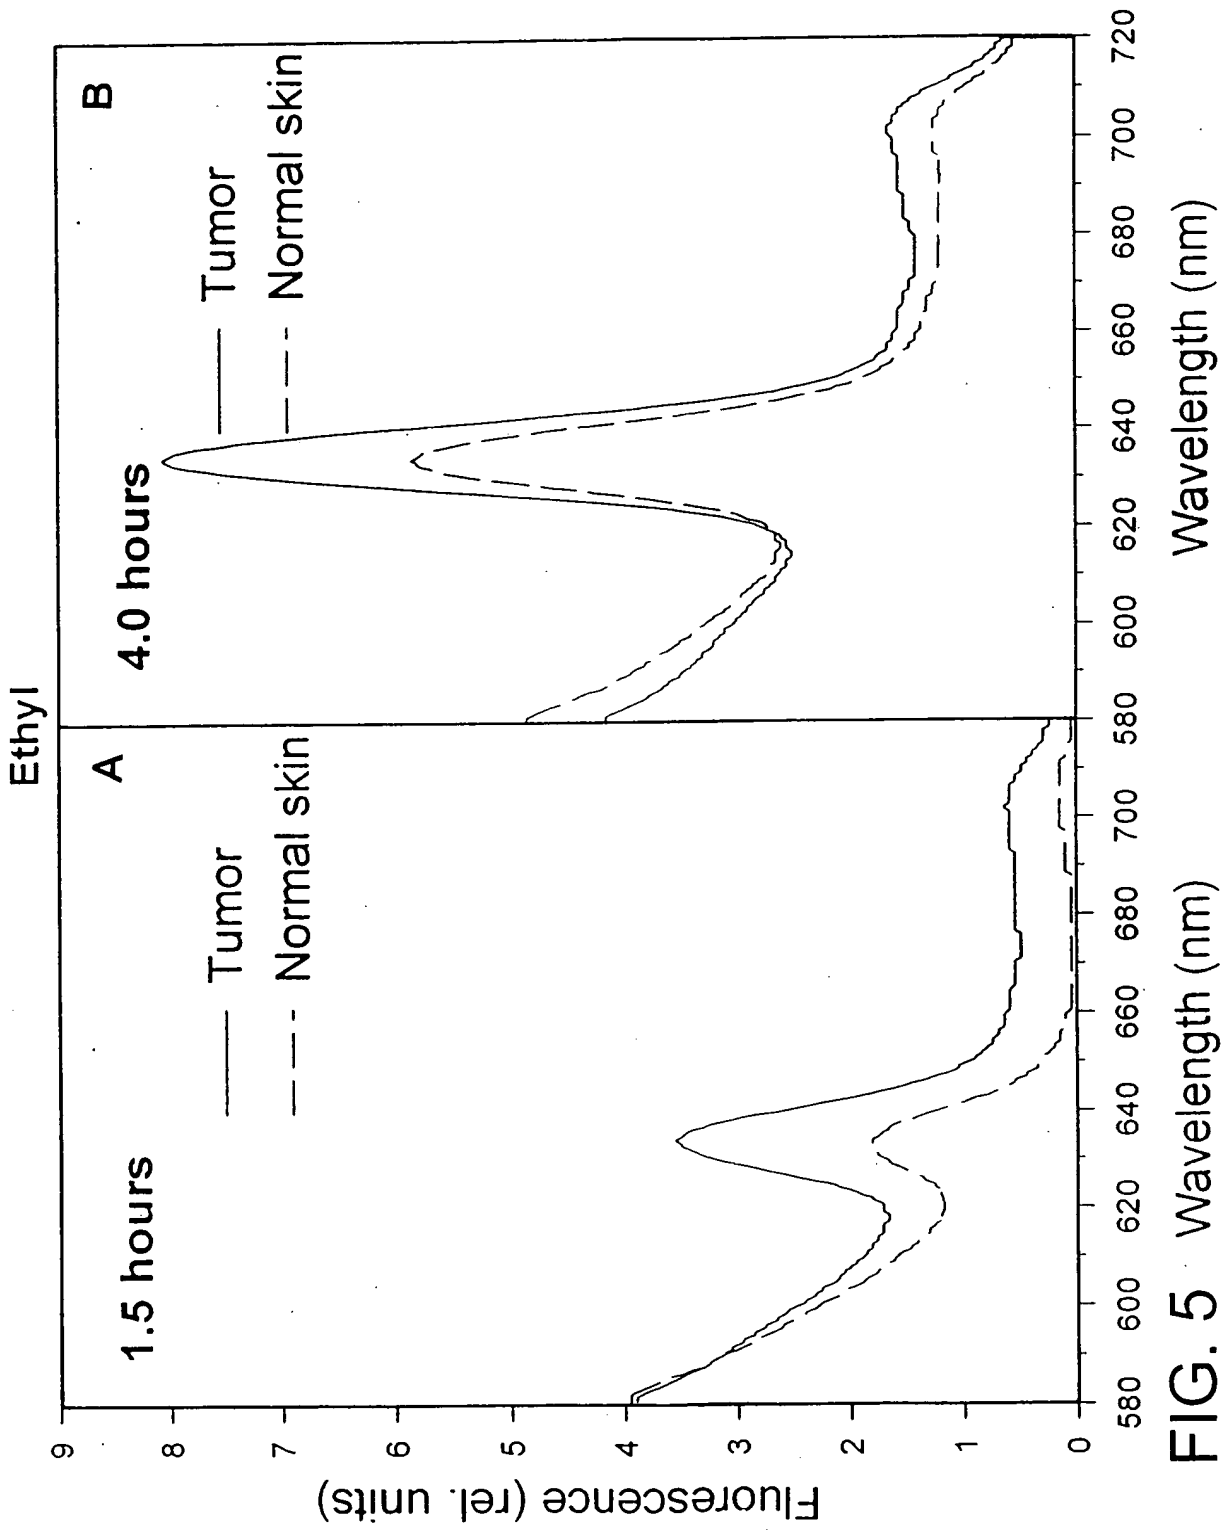


FIG. 4 Wavelength (nm)

**FIG. 5** Wavelength (nm)

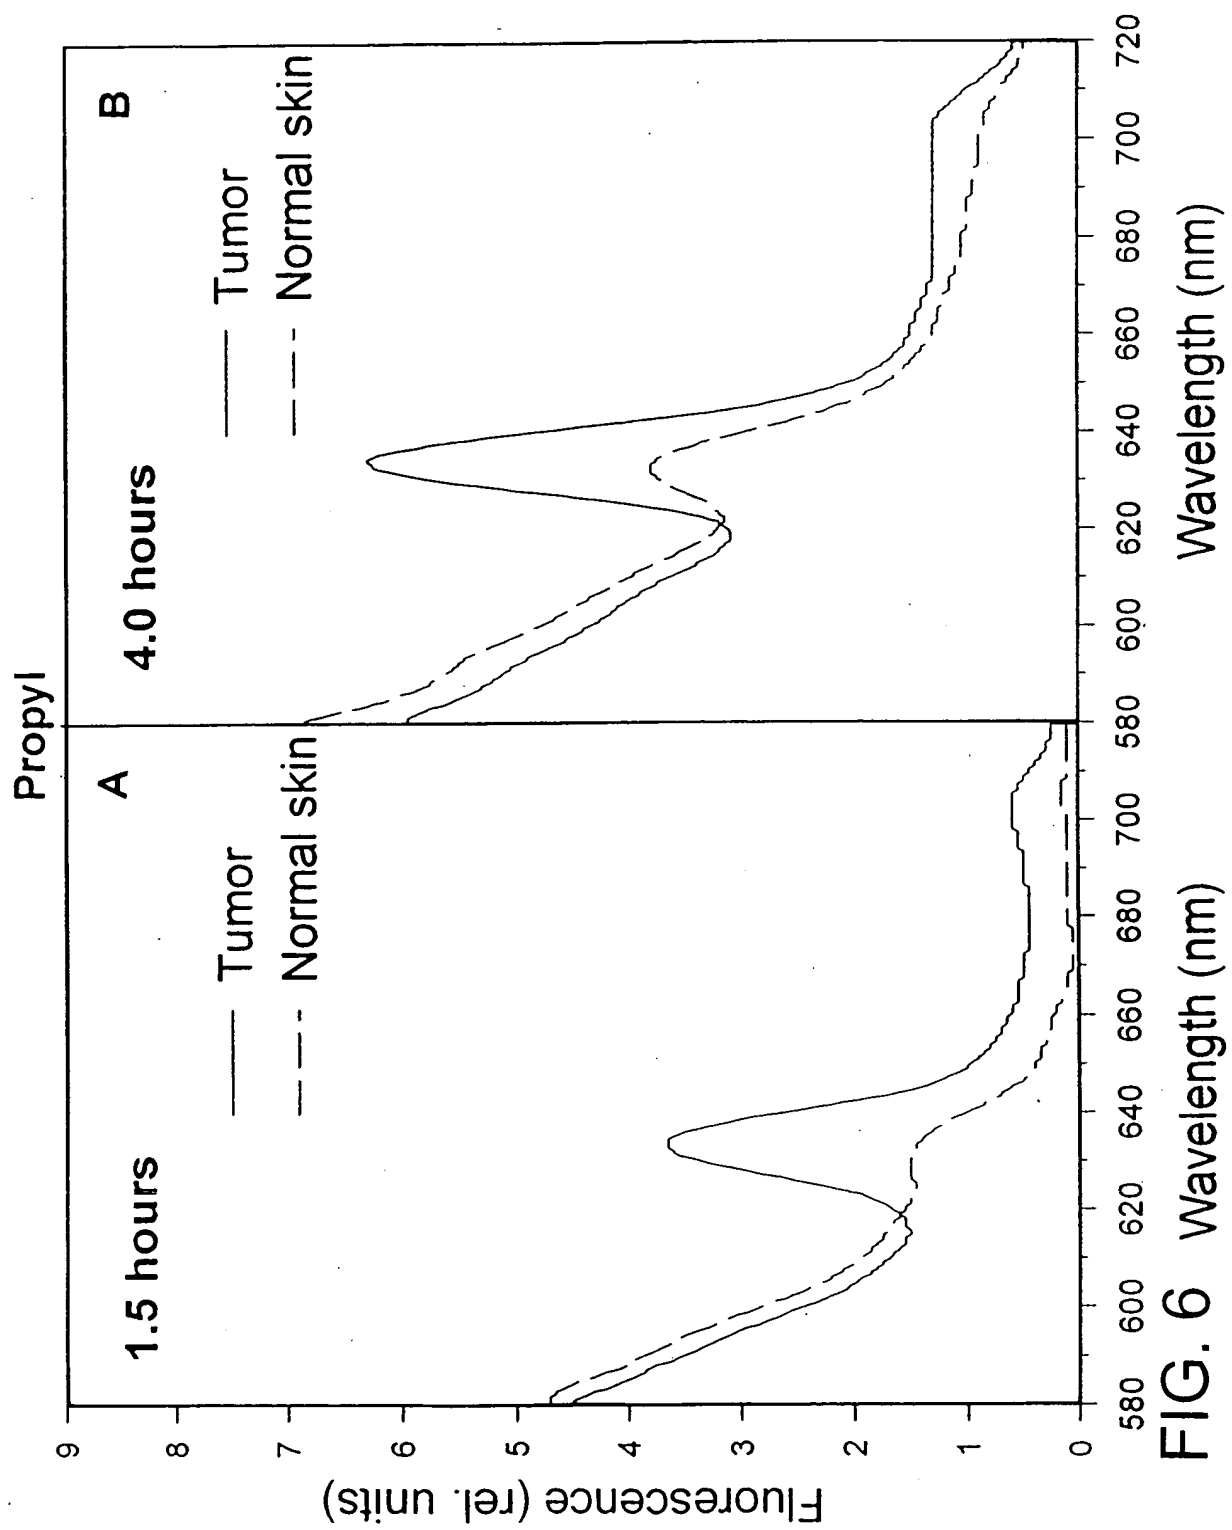


FIG. 6 Wavelength (nm)


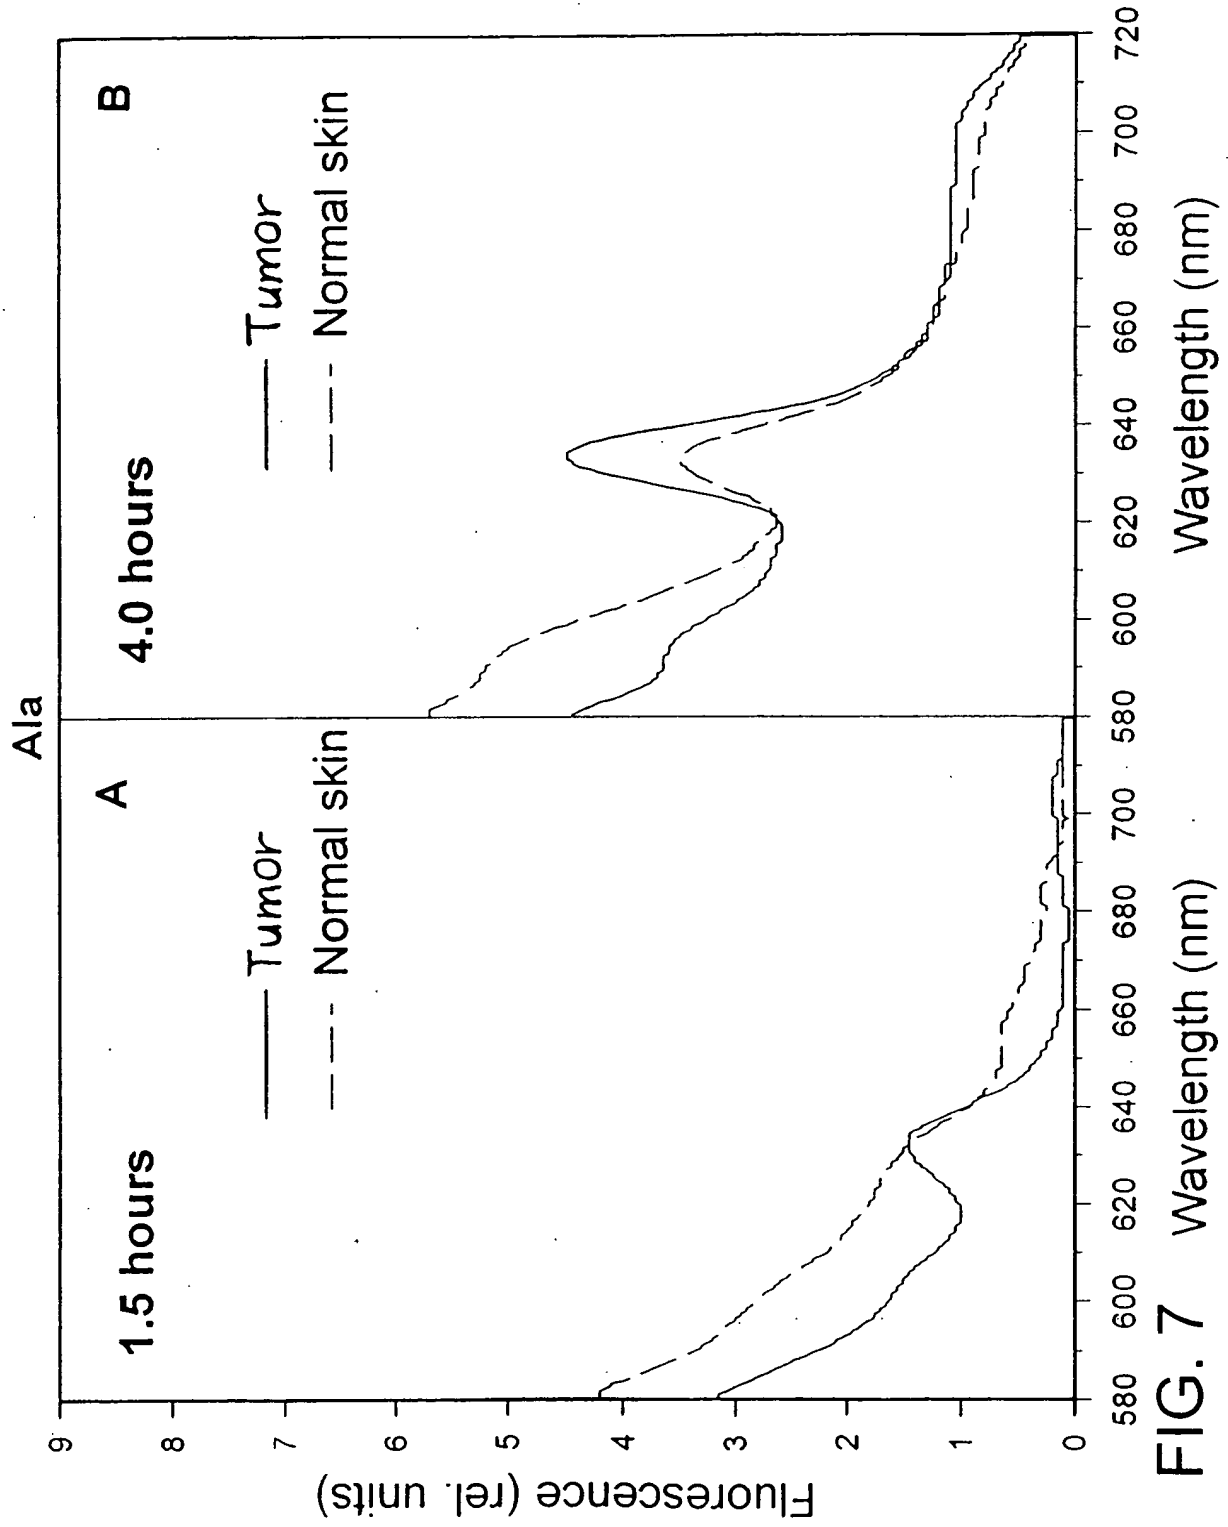
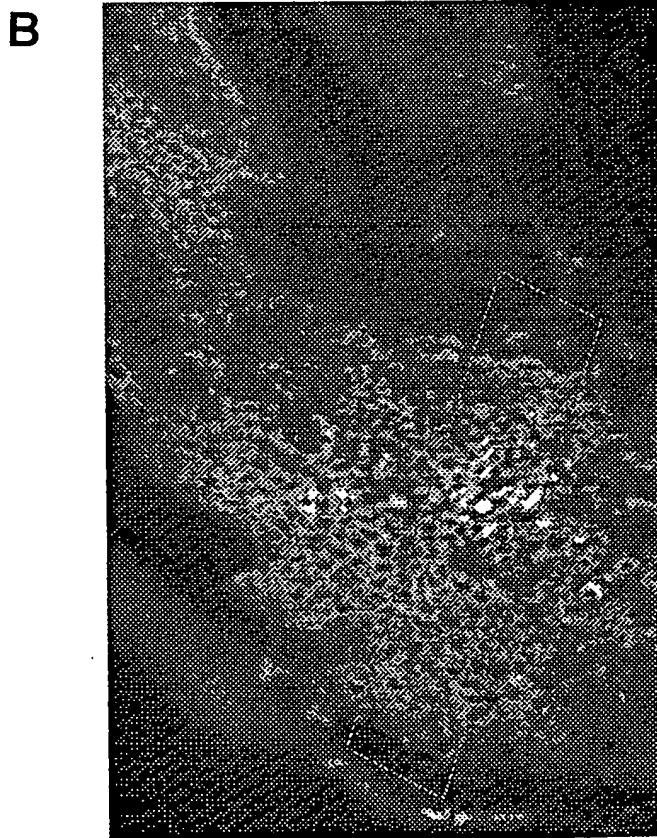


FIG. 7 Wavelength (nm)

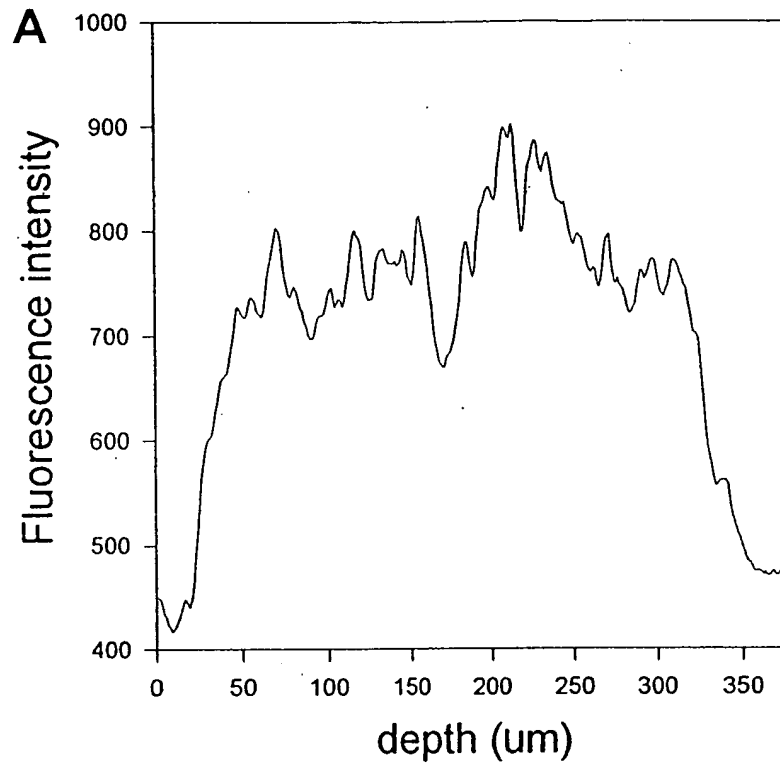

Free ALA
FIG. 8

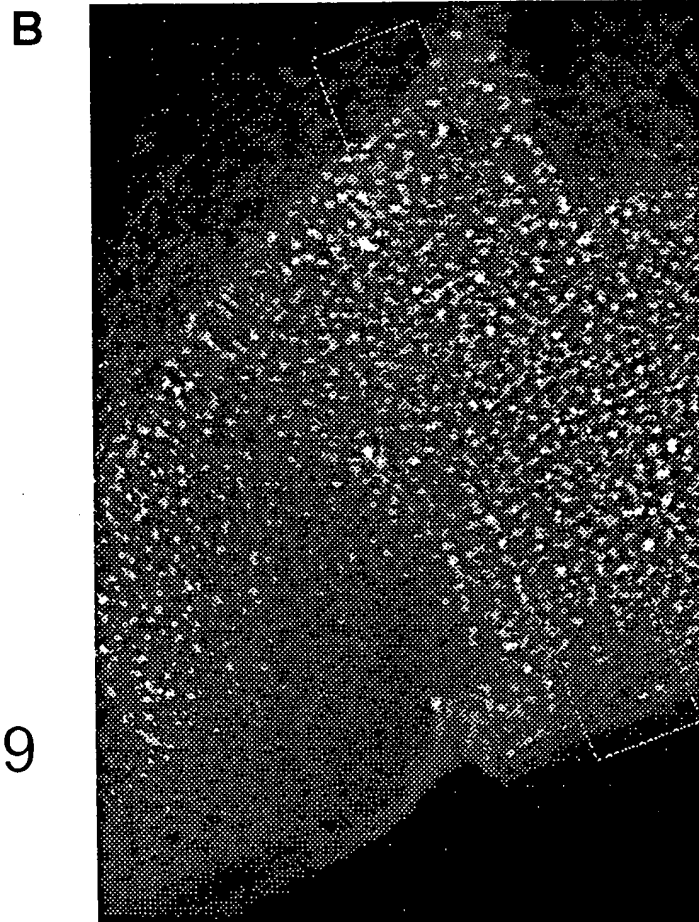
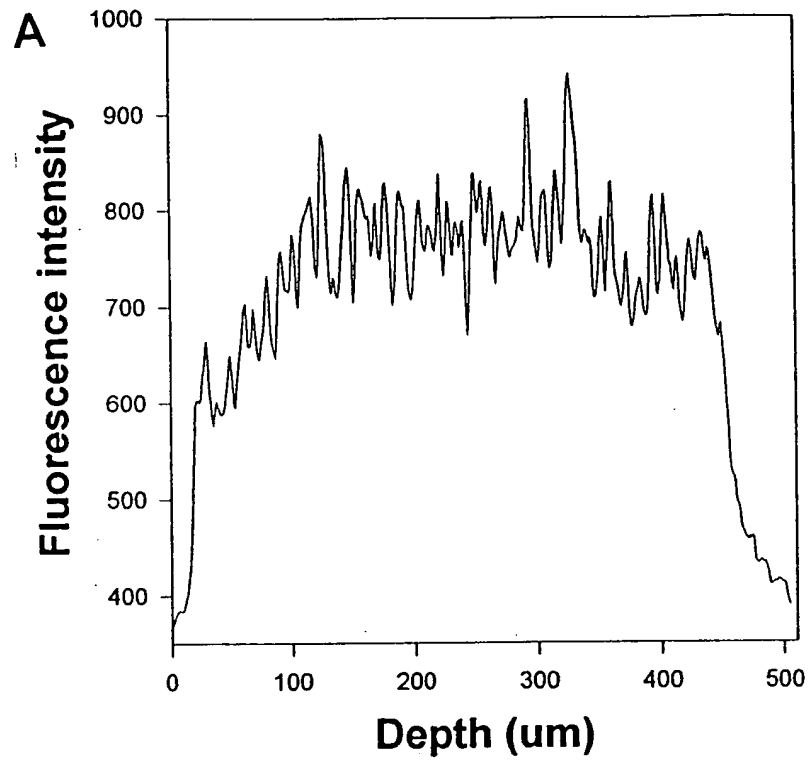
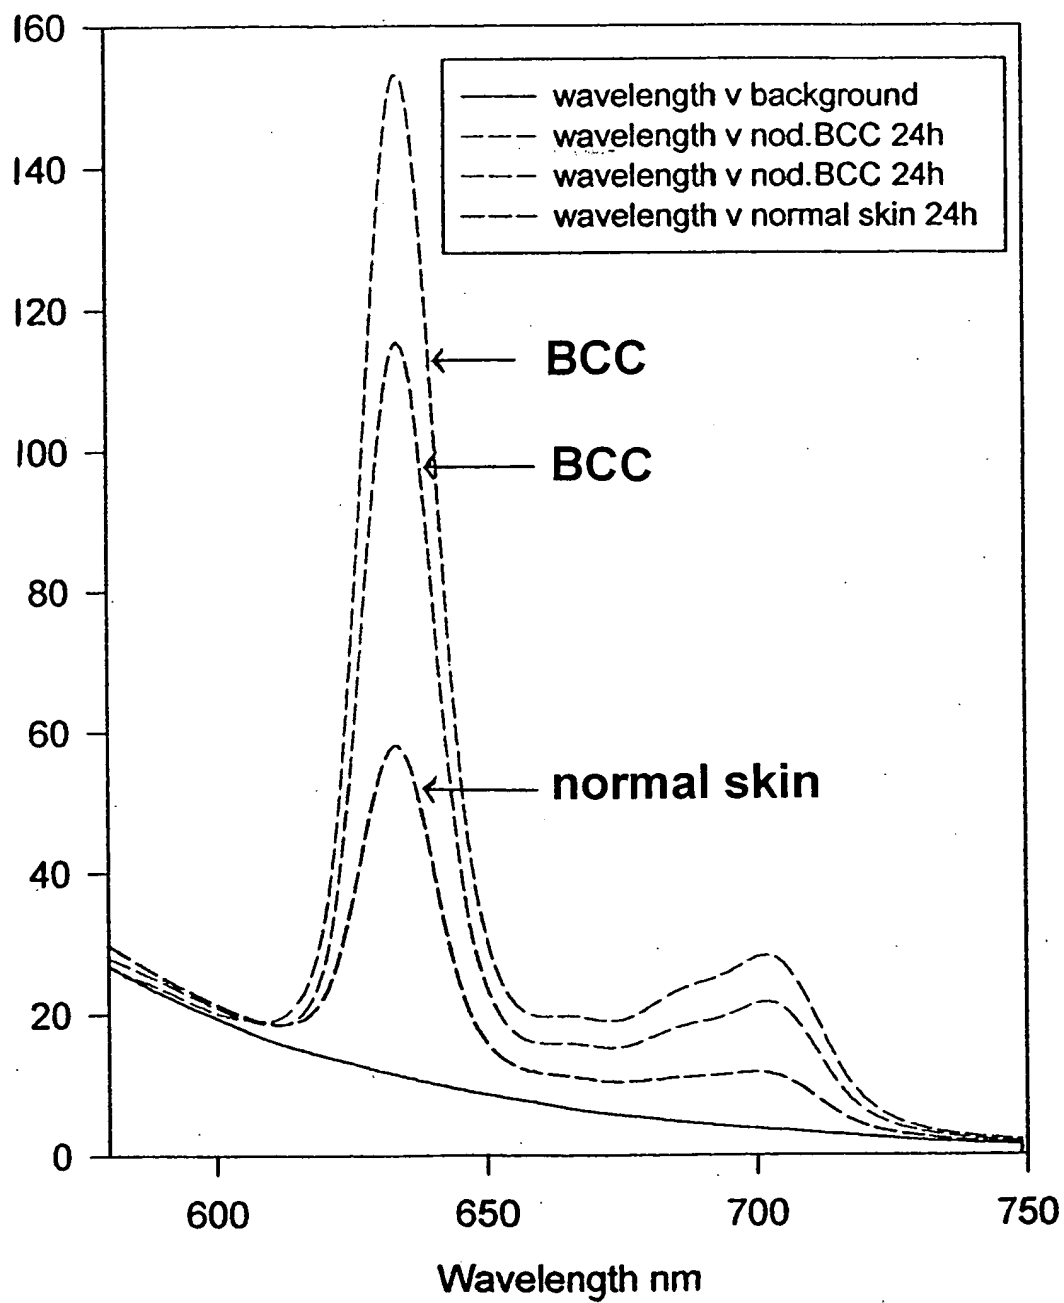
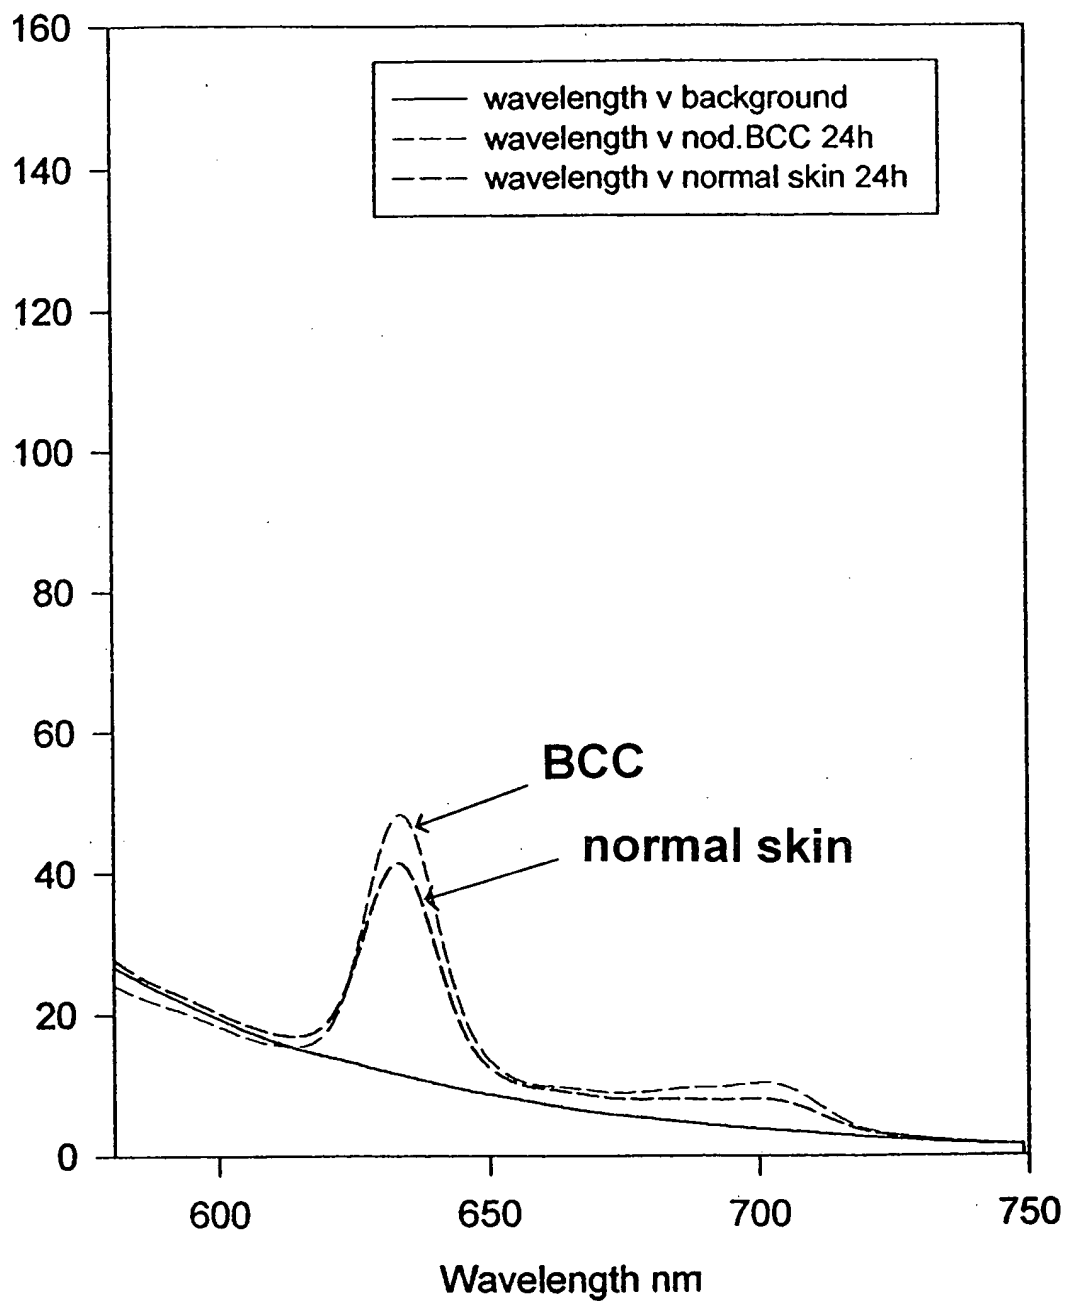


FIG. 9

ALA methylester

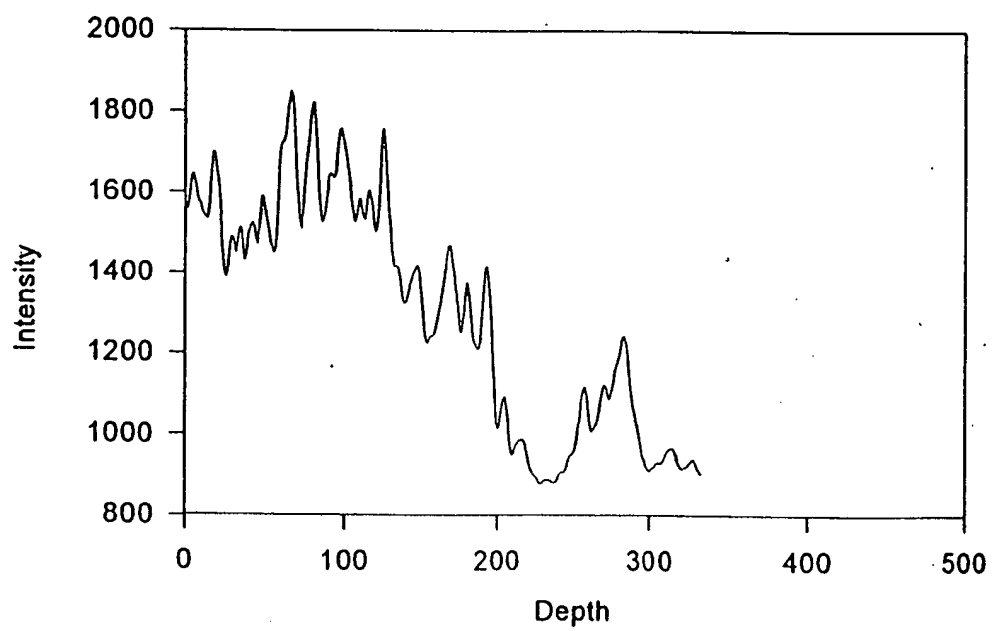
BCC ALA-methyl 24 hours**FIG. 10**

BCC ALA 24 hours**FIG. 11**

12 / 23

155-20

A



B

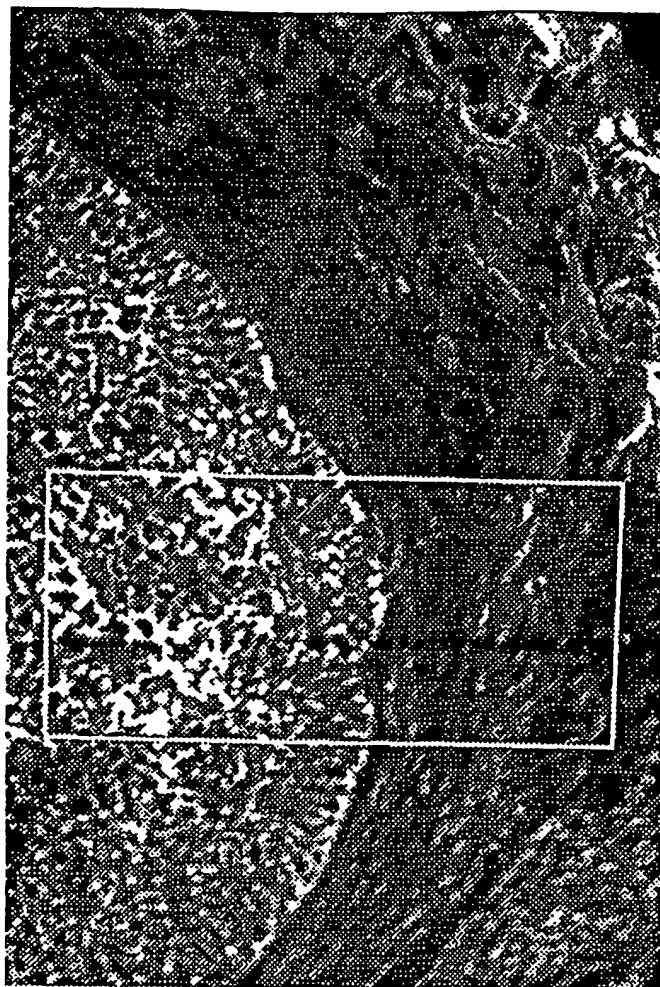


FIG. 12

156-1

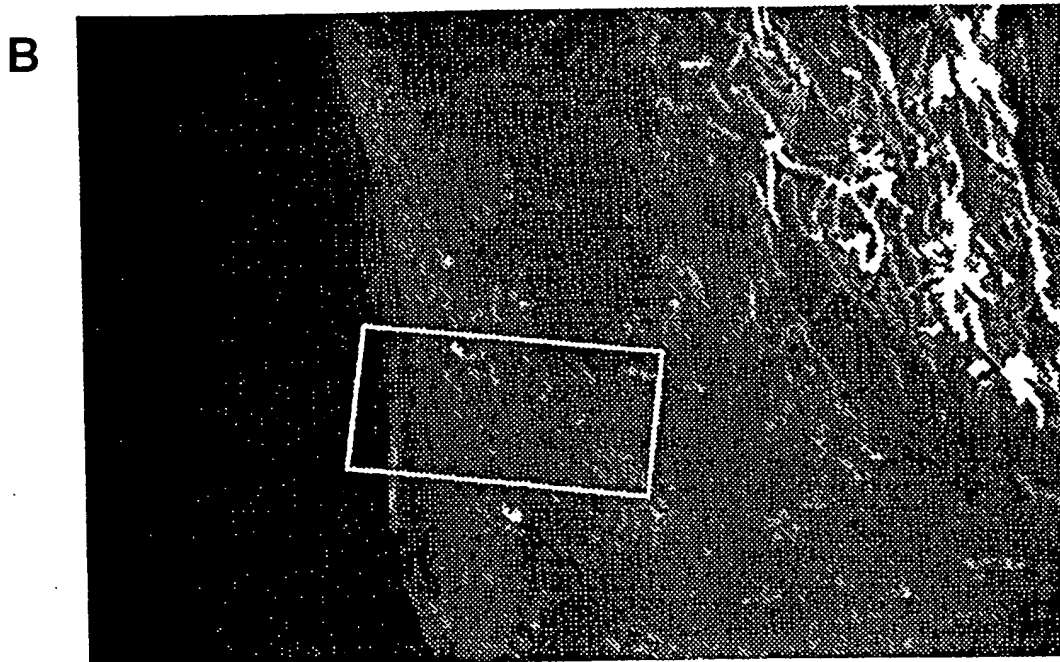
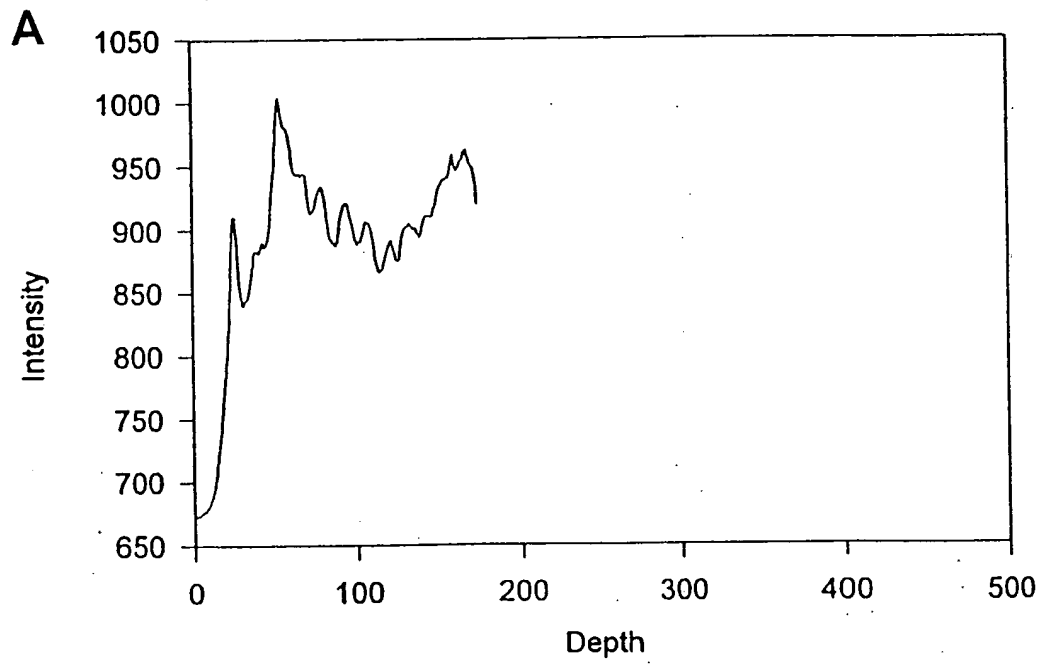


FIG. 13

153-11

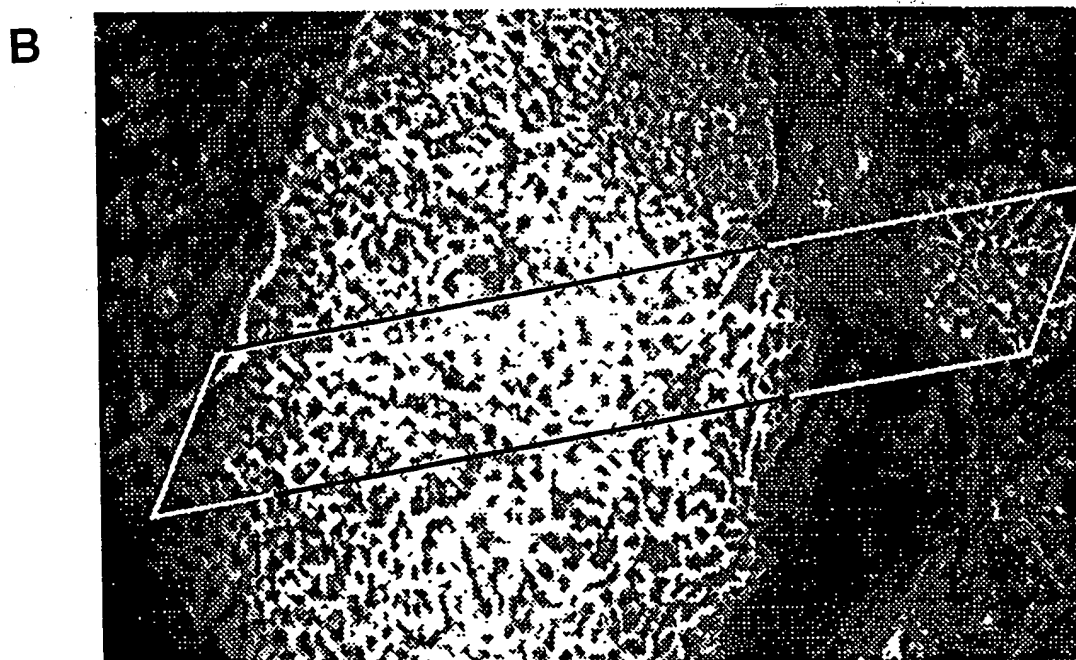
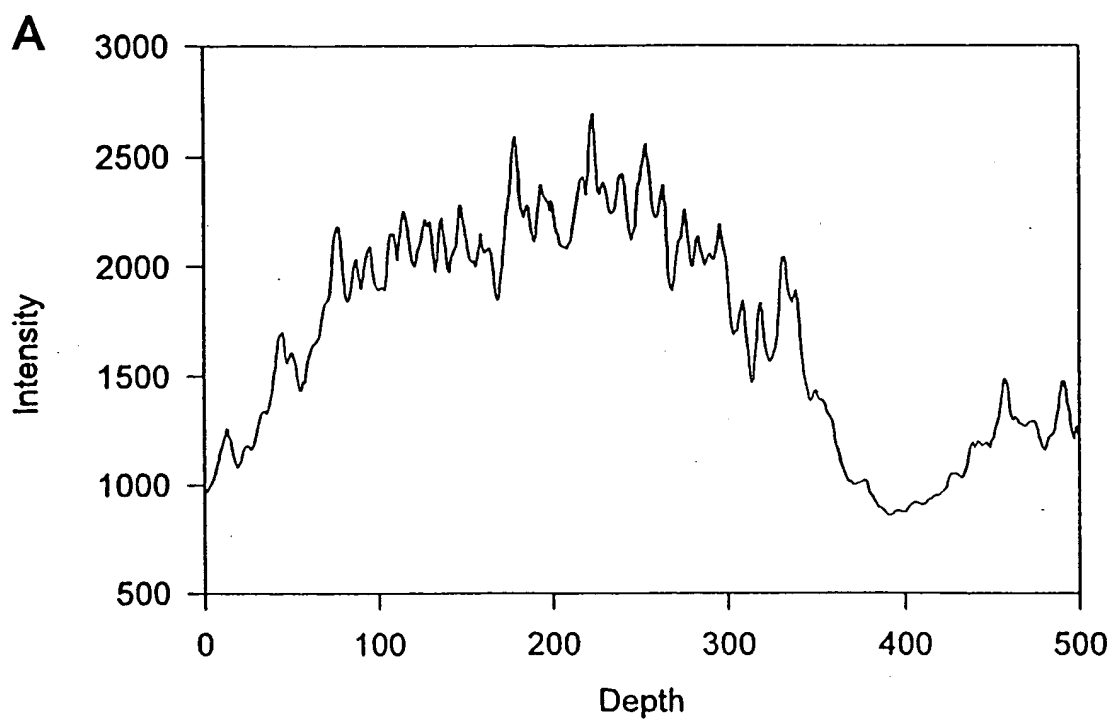


FIG. 14

158-1

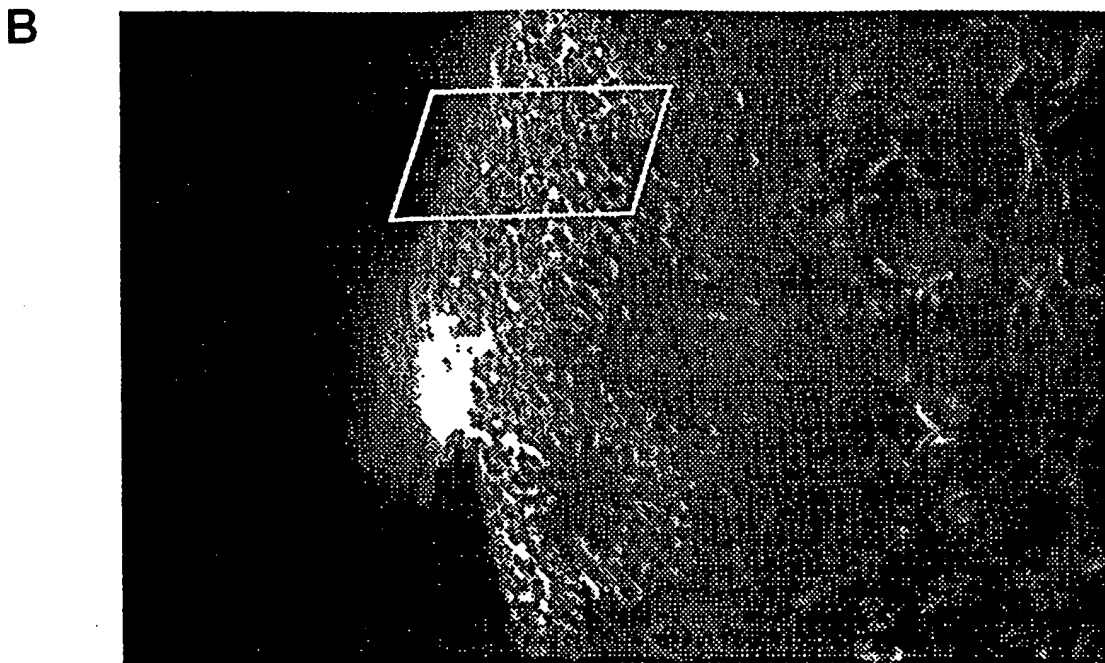
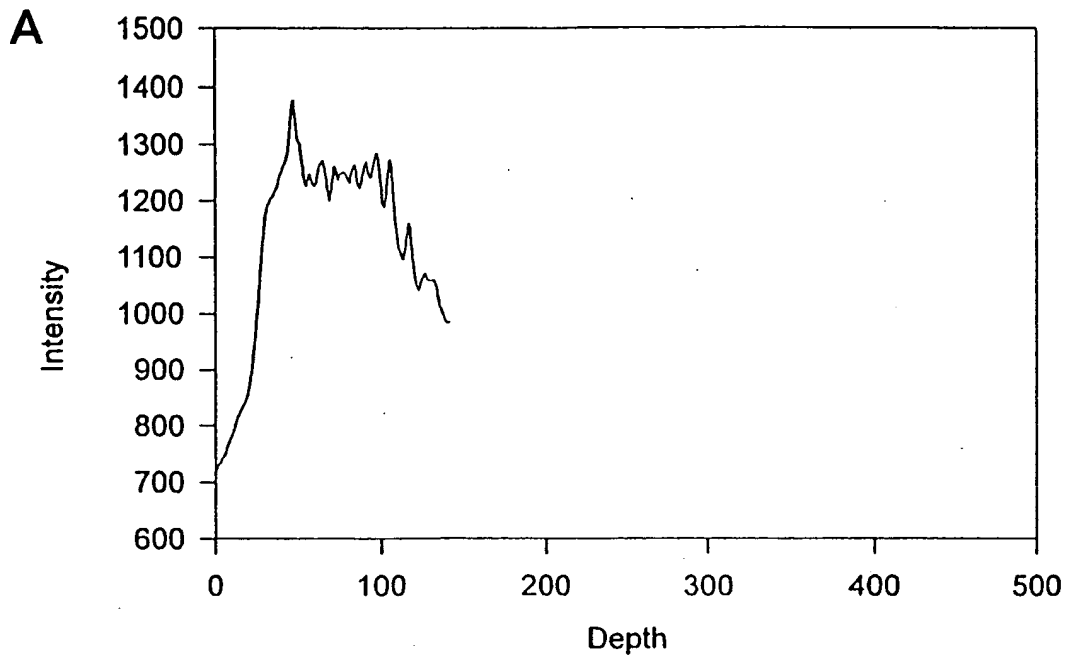


FIG. 15

159-4

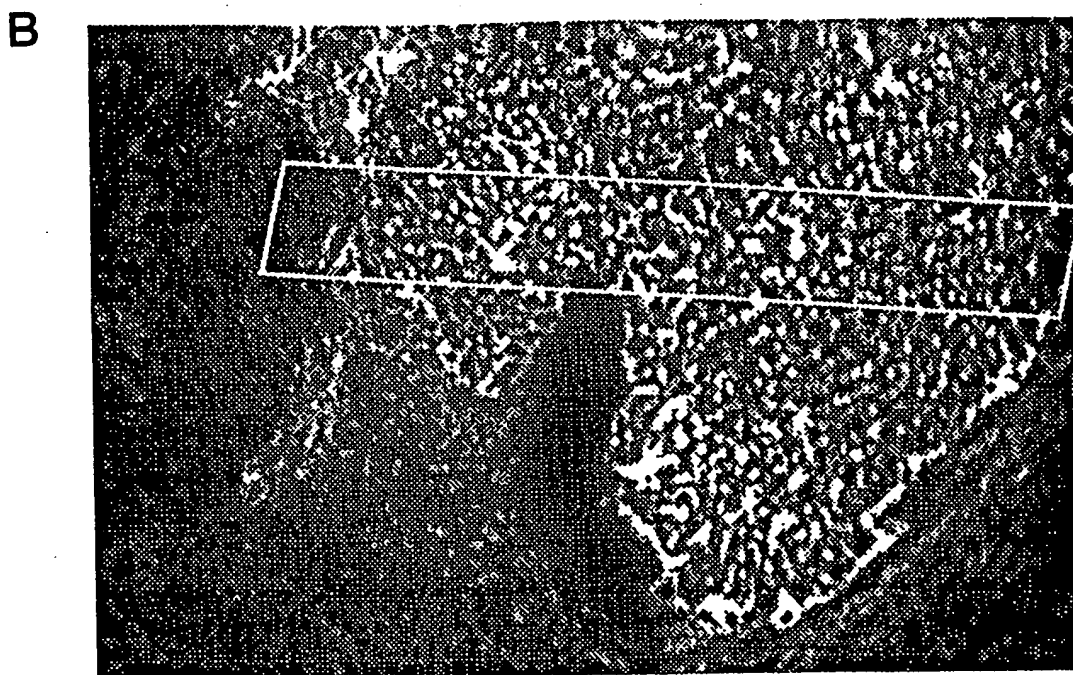
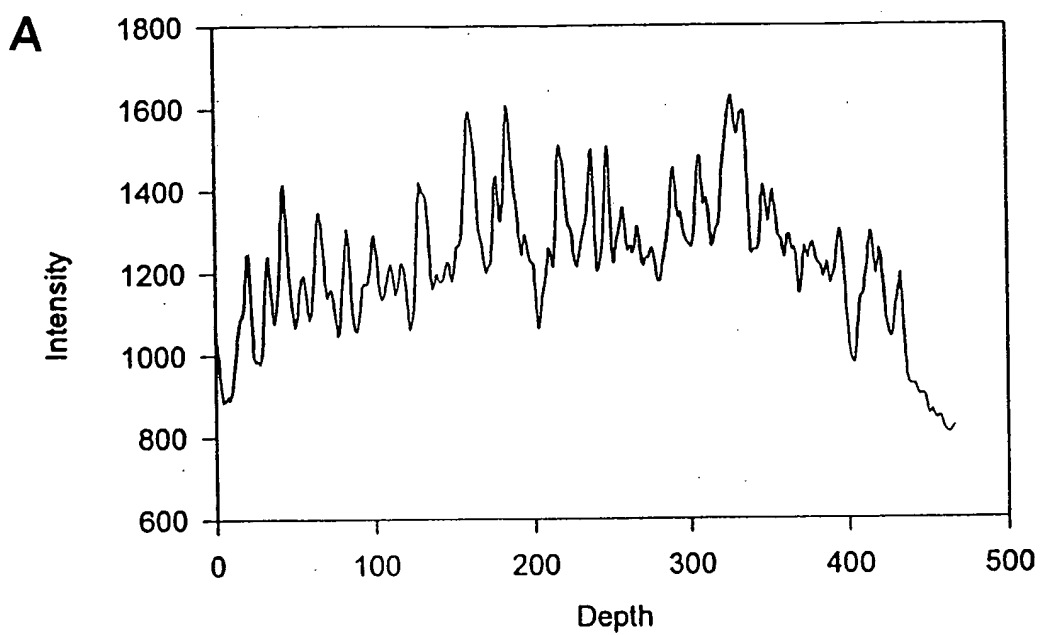


FIG. 16

160-1

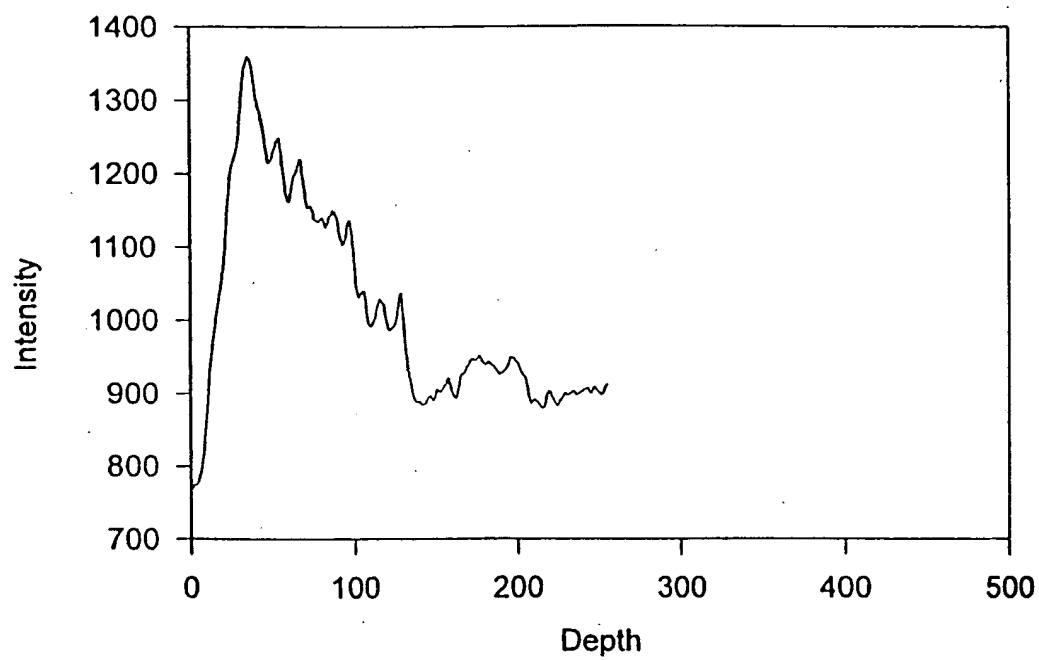
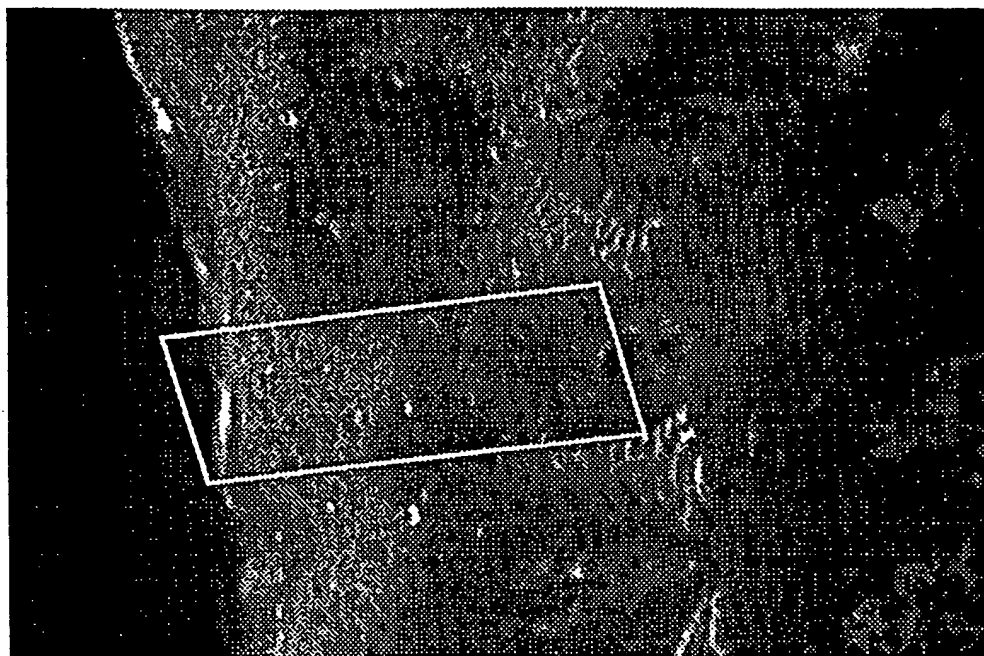
A**B**

FIG. 17

161-6

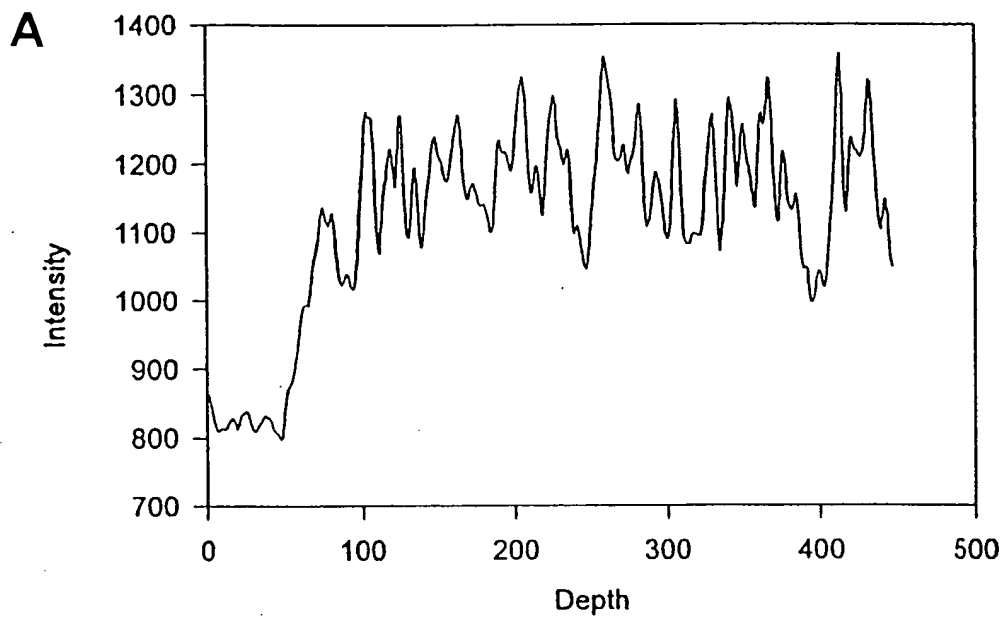
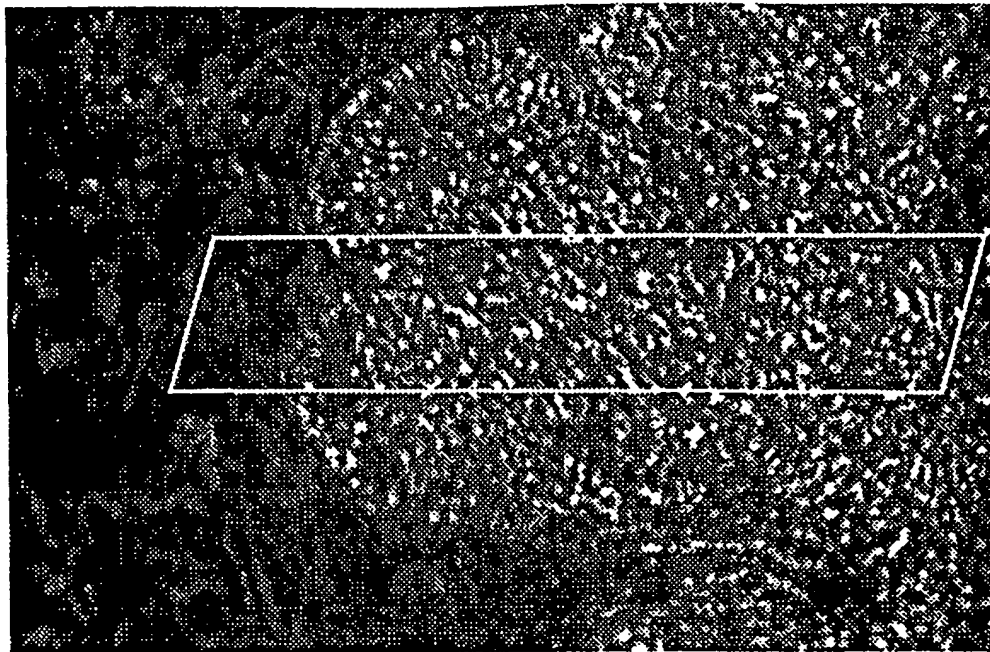
**B**

FIG. 18

162-1

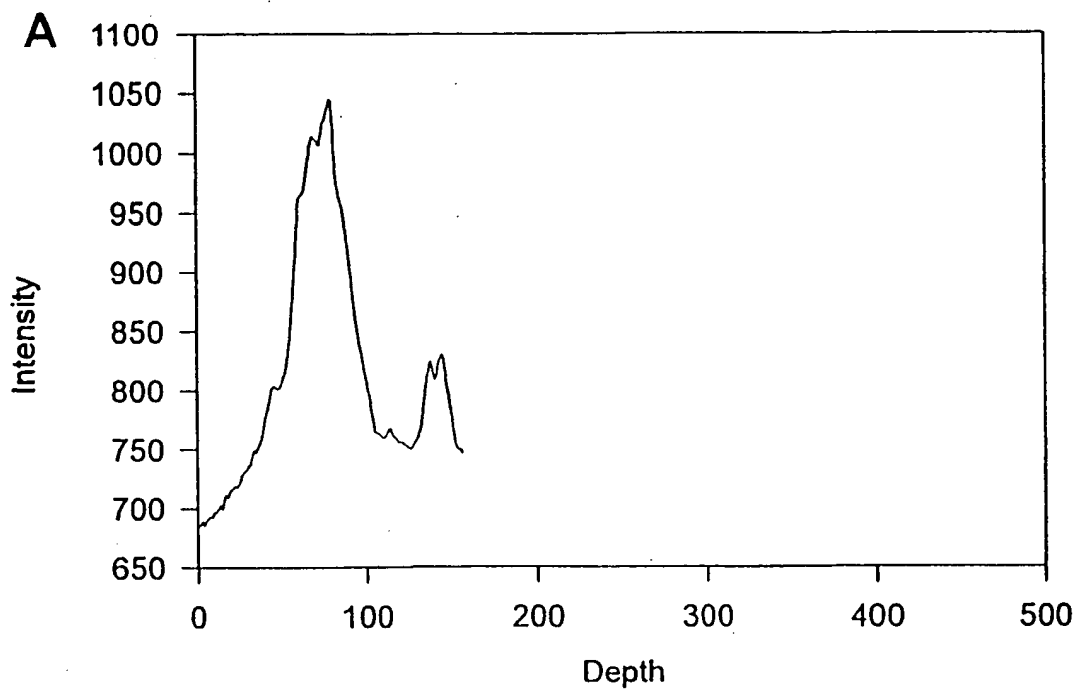
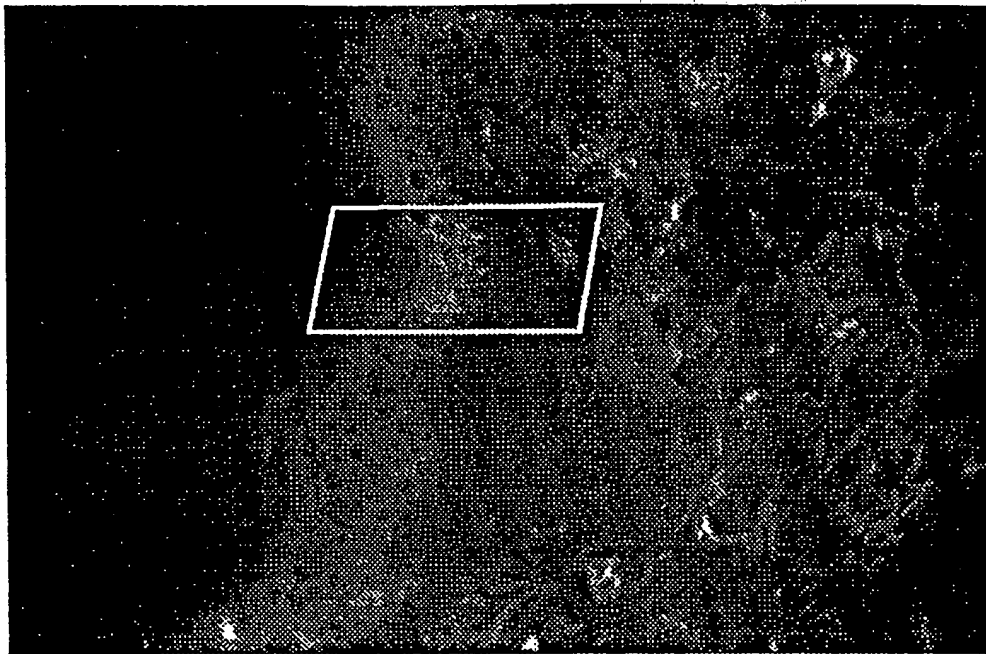
**B**

FIG. 19

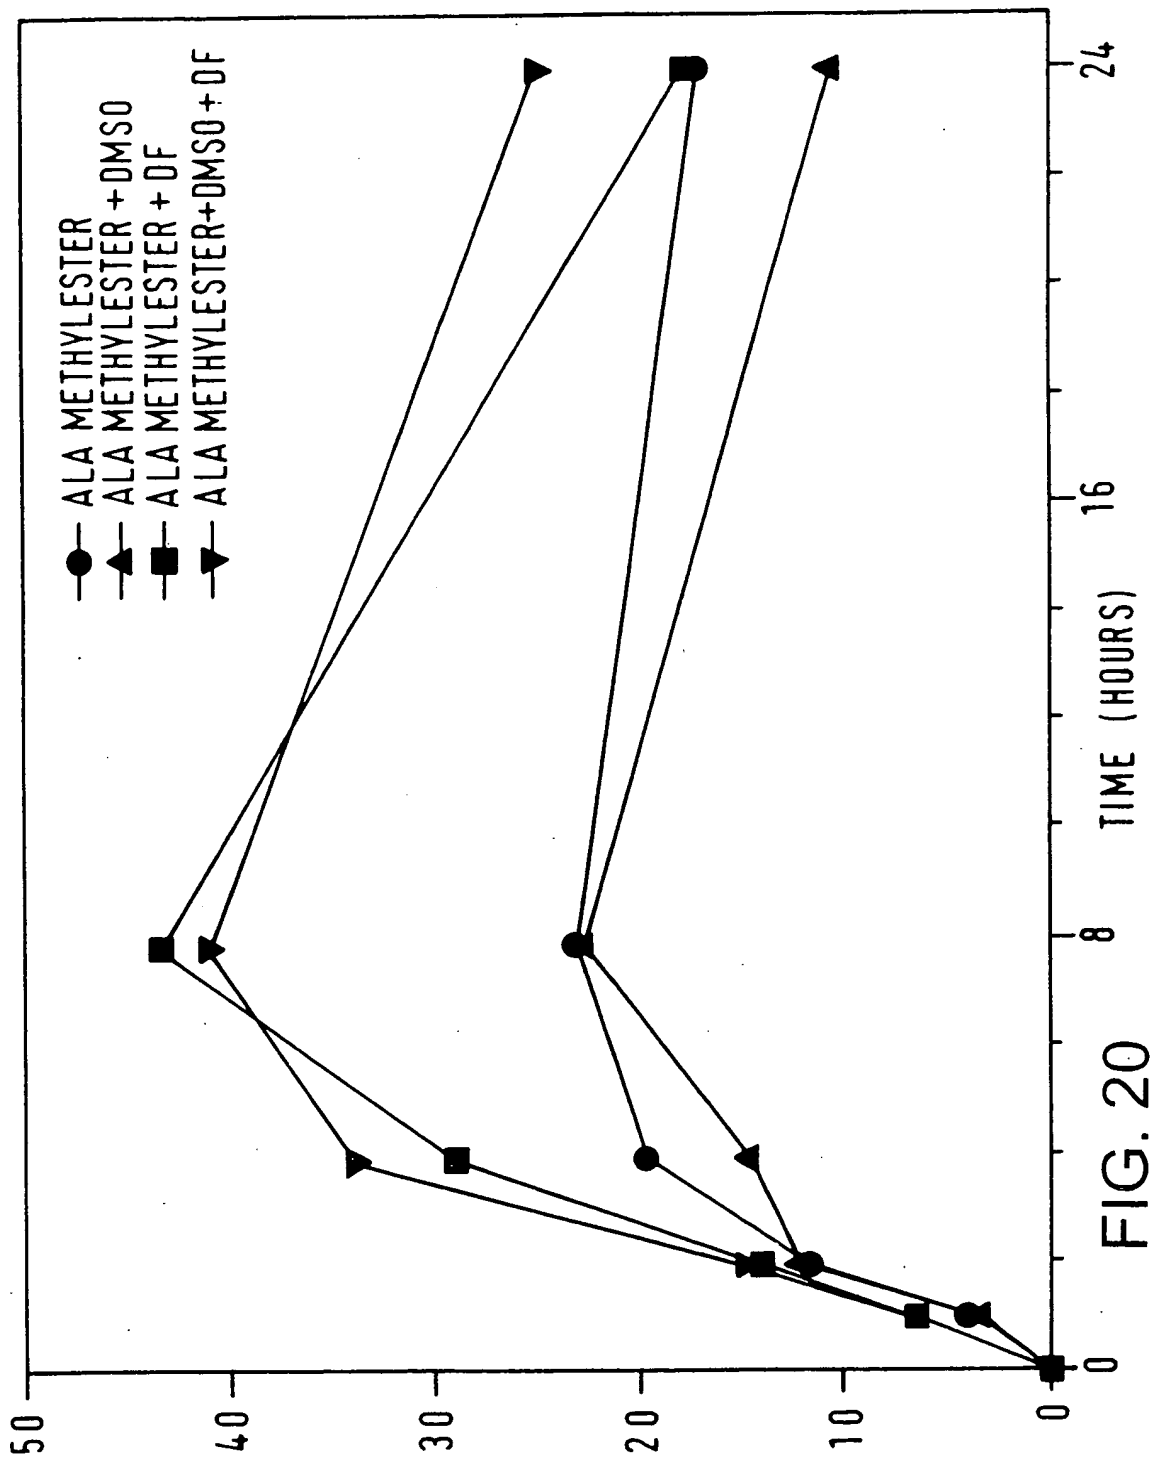


FIG. 20

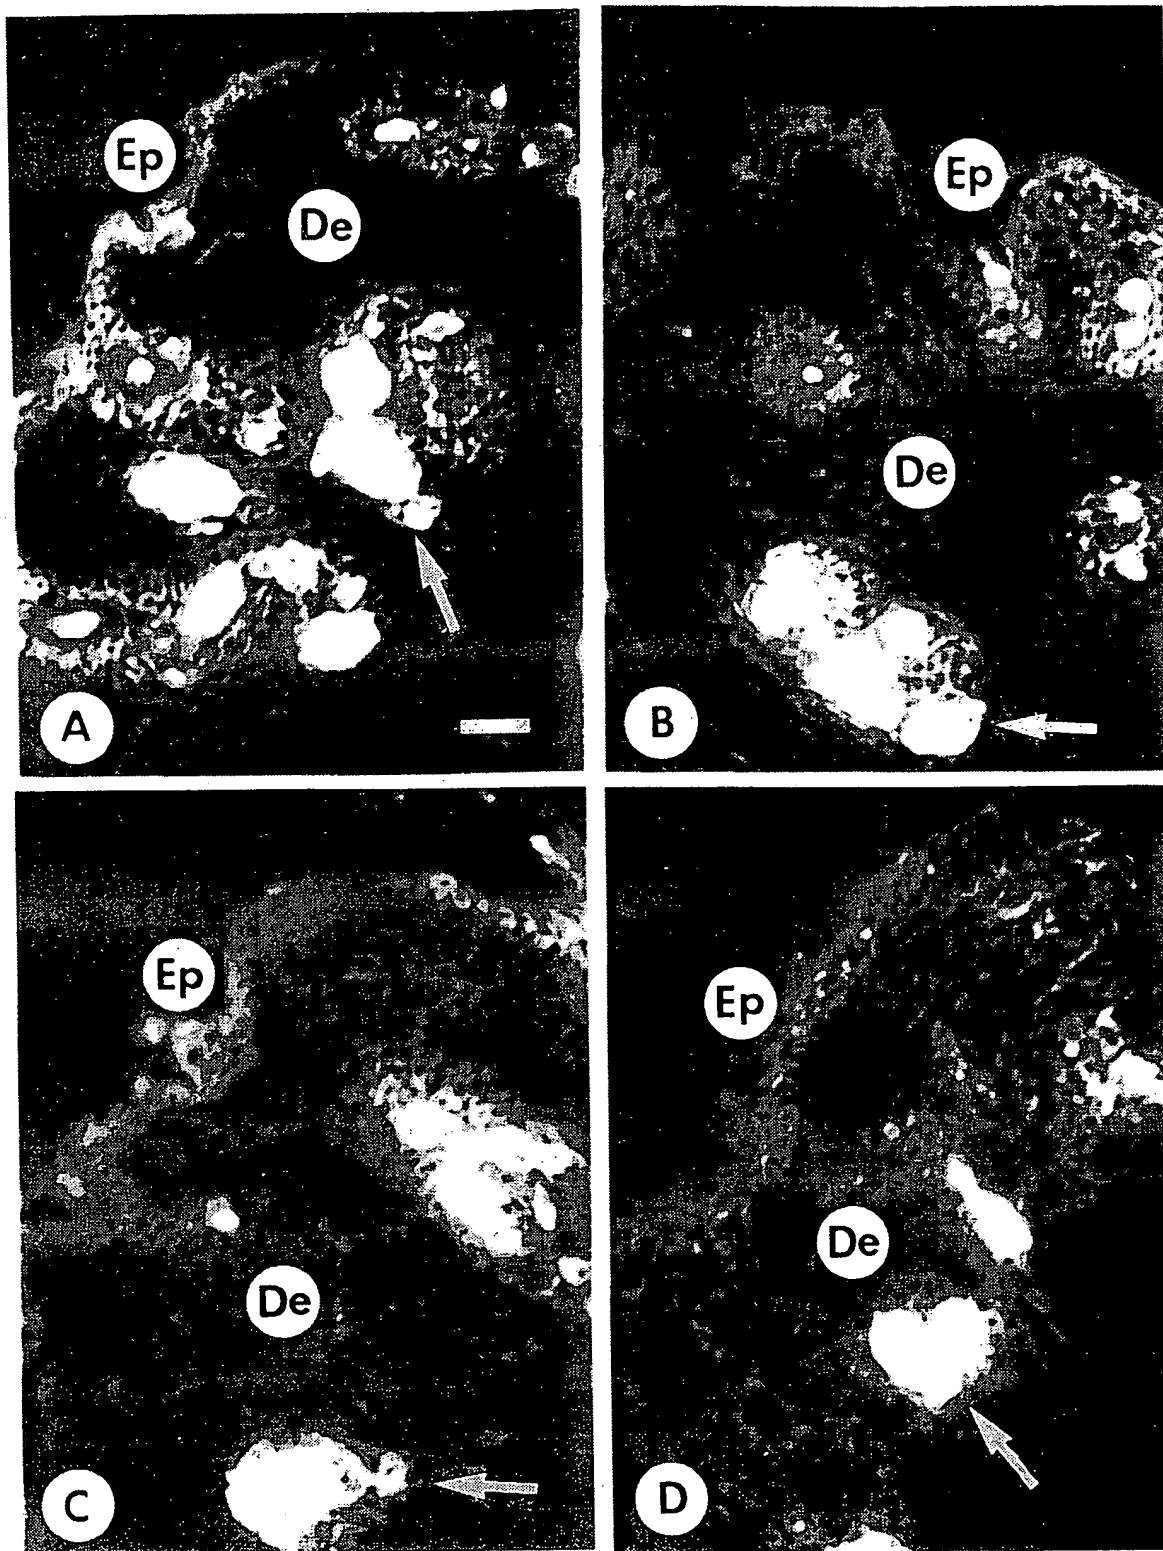


FIG. 21

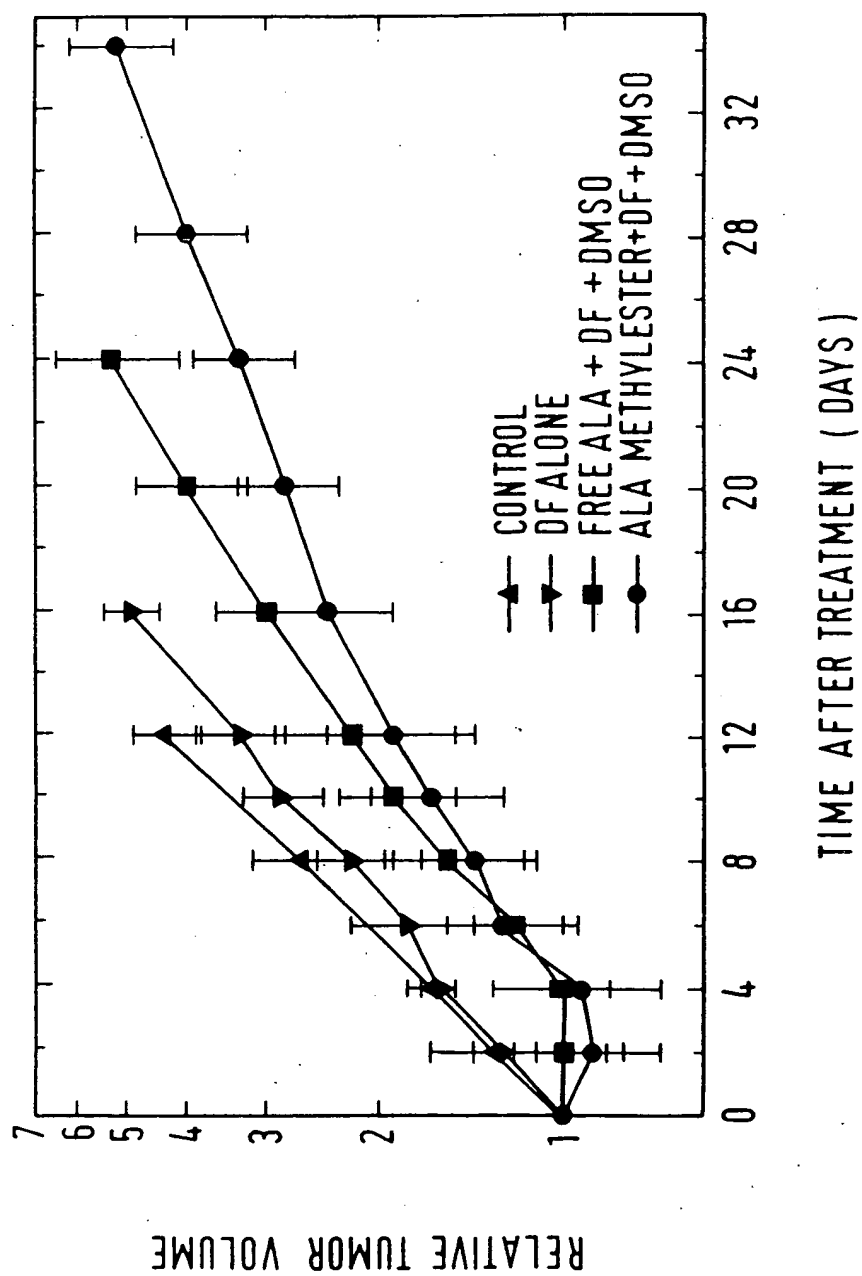


FIG. 22

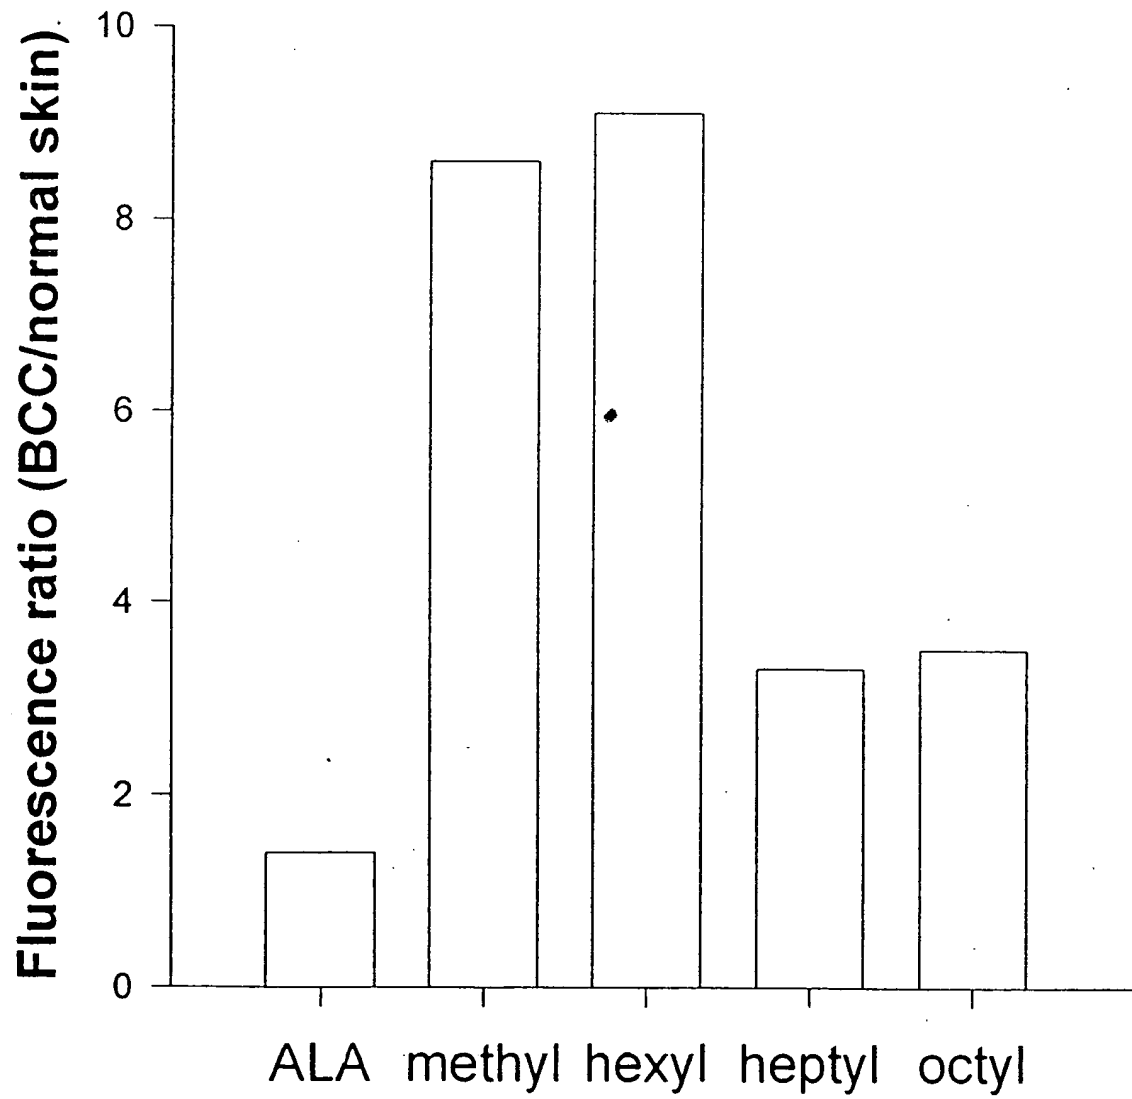


FIG. 23